

GELLER MICROANALYTICAL LABORATORY

426e BOSTON ST., TOPSFIELD, MA 01983-1216


TEL 978 887-7000 FAX 978-887-6671

Jg@gellermicro.com <http://www.gellermicro.com>


Certified to ISO-9001 & 17025

March, 2003

dPict32/CompMap - example

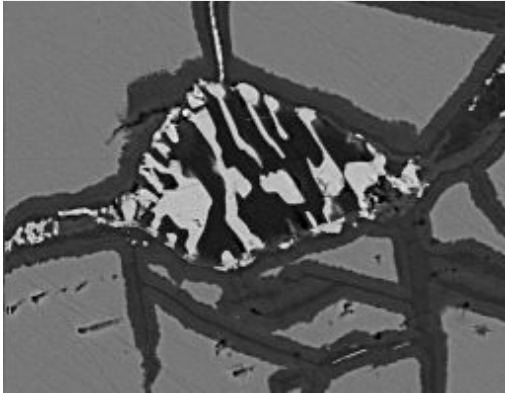

Backscattered electron image - Fayalite

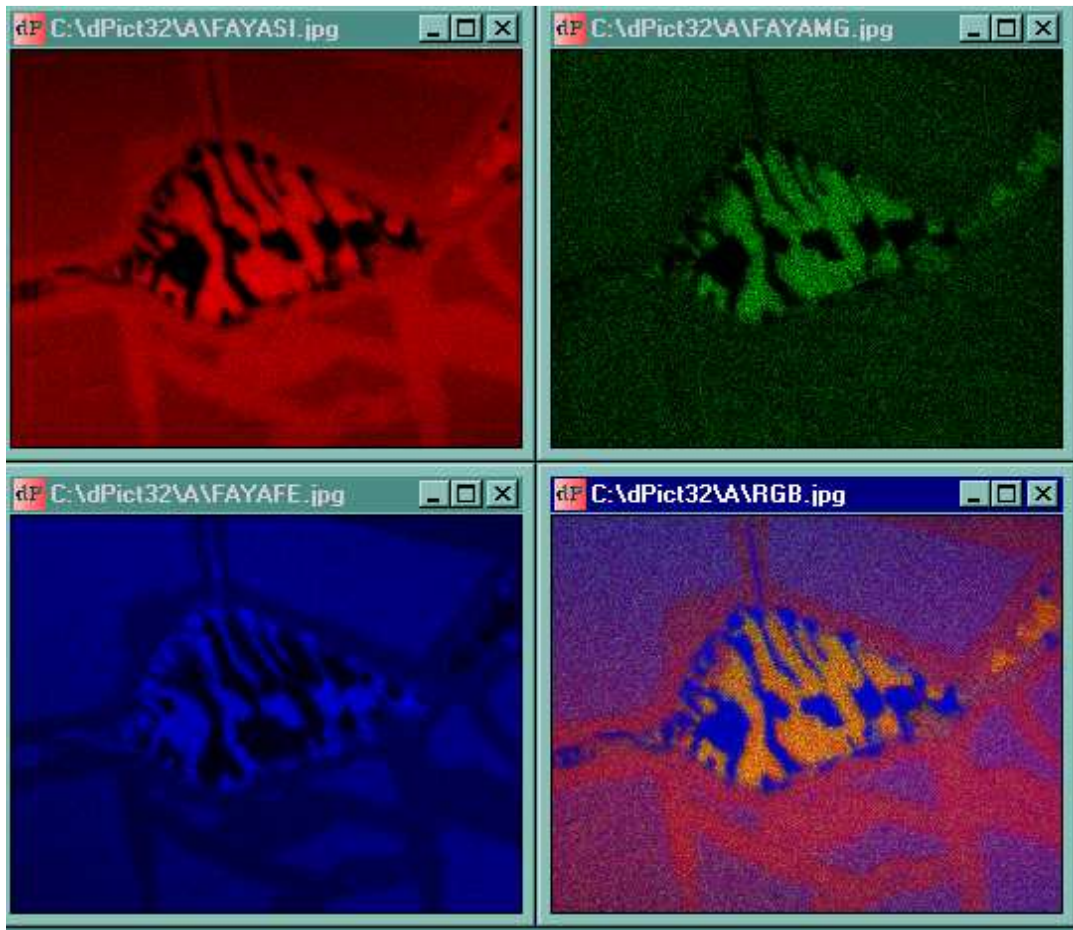

Top left – SiK α
Bottom left – FeK α

Top right - MgK α
Bottom right – RGB Log 3 band image